

EASYLYTE Na⁺/K⁺/Cl⁻/Ca⁺⁺/Li⁺ SOLUTIONS PACK

REF 2124 800mL

INTENDED USE

The EasyLyte Na⁺/K⁺/Cl⁻/Ca⁺⁺/Li⁺ Solutions Pack is intended for the quantitative determination of sodium (Na⁺), potassium (K⁺), chloride (Cl⁻), calcium (Ca⁺⁺) and lithium (Li⁺) in human serum, plasma, whole blood and urine (urine results for Na⁺, K⁺ and Cl⁻ only) using the MEDICA EasyLyte® Analyzer.

For professional use only. For *in vitro* diagnostic use only.

SUMMARY AND EXPLANATION

Electrolyte measurements in biological fluids were traditionally performed using flame photometry. The development of selective organic compounds for sodium, potassium, chloride, calcium and lithium and other electrolytes has permitted the development of sensors capable of the direct measurement of biological fluids throughout the physiological range. These sensors are known as ion-selective sensors.

Sodium is the major cation in extracellular fluid and has a major effect on osmotic pressure and water distribution between cells, plasma and interstitial fluid. Low sodium imbalance (Hyponatremia) is associated with diarrhea, server polyuria, metabolic acidosis, Addison's disease and renal tubular disease. High sodium imbalance (Hypernatremia) is associated with hyperadrenalism, severe dehydration, brain injury, diabetic coma and excess treatment with sodium salts.

Potassium is a major cation in intracellular liquid. Potassium imbalance has a direct effect on muscle irritability, myocardial function and respiration. Some conditions that effect potassium levels in blood include hypoaldosternism, diarrhea, vomiting and therapy with diuretics for hypertension or cardiac disease. Unlike sodium, there is no mechanism to maintain a threshold potassium level in the body.

Chloride is the major extracellular anion and it has a direct effect on osmotic pressure, water distribution and anion-cation imbalance. Low chloride levels are caused by chronic pyelonephritis, Addisonian crisis, metabolic acidosis and prolonged vomiting. High chloride levels are observed in dehydration, congestive heart failure, hyperparathyroidism and extensive treatment with or intake of chloride.

Ionized calcium is the only physiologically active form of calcium. Increased or decreased levels of ionized calcium are directly related to hyperparathyroidism and hypoparathyroidism respectively. Calcium regulates muscle contraction, hormone secretion and membrane permeability. Acidosis (low pH) causes an increase in the amount of ionized calcium and alkalosis (high pH) causes a decrease in the amount of ionized calcium.

Lithium is not present in healthy people and it is not metabolized. However it is administered in the form of a carbonate salt to control manic-depressive disorders. It is believed that lithium medications affect the central nervous system neurotransmitters, as well as the kidneys. Excessive levels of lithium may cause lithium toxicity.

PRINCIPLE OF THE PROCEDURE

The EasyLyte analyzer measures sodium, potassium, chloride, calcium and lithium in human serum, plasma, whole blood and urine (for Na⁺, K⁺ and Cl⁻ only) using ion-selective electrode technology. The flow-through sodium electrode uses a selective membrane that is specially formulated to be sensitive to sodium ions. The potassium, chloride, calcium and lithium electrodes employ a similar design with appropriate selective membrane materials. The potential of each electrode is measured relative to a fixed and stable voltage that is established by the double-junction silver/silver chloride reference electrode. An ion-selective electrode develops a voltage that varies with the concentration of the ion to which it responds. The relationship between the voltage developed and the concentration of the sensed ion is logarithmic, as expressed by the Nerst equation:

$$E = E^{\circ} + \frac{RT}{nF} \log (g C)$$

where: E = The potential of the electrode in sample solution
 E° = The potential developed under standard conditions
 RT/nF = A temperature dependent "constant", termed the slope(s)
 n = 1 for sodium, potassium, chloride, lithium
 n = 2 for calcium
 Log = Base ten logarithm function
 g = Activity coefficient of the measured ion in the solution
 C = Concentration of the measured ion in the solution

REAGENTS

800mL Solutions Pack (REF 2124)

Standard A Solution, 800mL

140.0 mmol/L Na^+
 4.0 mmol/L K^+
 125.0 mmol/L Cl^-
 1.25 mmol/L Ca^{++}
 1.00 mmol/L Li^+
 Buffer
 Preservative
 Wetting Agent

Standard B Solution, 180mL

35.0 mmol/L Na^+
 16.0 mmol/L K^+
 41.0 mmol/L Cl^-
 2.50 mmol/L Ca^{++}
 0.40 mmol/L Li^+
 Buffer
 Preservative
 Wetting Agent

Wash Solution, 80mL

0.1 mol/L Ammonium bifluoride

Waste Container

PRECAUTIONARY STATEMENTS



May cause skin irritation (H315)

May cause eye irritation (H319)

If on skin, wash with plenty of soap and water (P302 + P352)

If in eyes, rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do, and continue rinsing. (P305 + P351 + P338)



When used, the Solutions Pack contains human body fluids and is considered biohazardous. Handle and dispose of the Solutions Pack using the same precautions as with any biohazardous material. Discard according to local regulations.

INSTRUCTIONS FOR SOLUTIONS PACK HANDLING, STORAGE AND STABILITY


The Solutions Pack is ready to use as supplied. Unopened, the Solutions Pack is stable until the expiration date listed on the label if stored at 4–25°C. After installation, the Solutions Pack is stable on-board the EasyLyte analyzer until the expiration date listed on the label. DO NOT FREEZE.

REMOVAL OF USED SOLUTIONS PACK

Following standard laboratory precautions, grasp the Solutions Pack firmly and pull away from the analyzer. DO NOT SQUEEZE SOLUTIONS PACK. Place the red cap over the four connectors and discard according to local regulations.


INSTALLATION OF NEW SOLUTIONS PACK

Remove the new Solutions Pack from the shipping container. Remove the orange label, record the date on the tear off tab and affix to the front of the Solutions Pack. This records the Solutions Pack installation date. Remove the red cap. Install the new Solutions Pack until it fits firmly into the solutions valve.

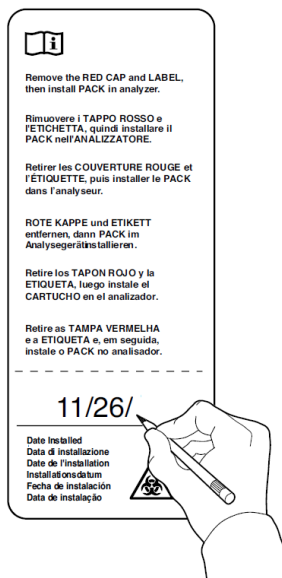

RESET COUNTER INSTRUCTIONS

The EasyLyte analyzer has an internal counter which keeps track of the Solutions Pack usage. The % counter must be set to zero (0) each time a new Solutions Pack is installed. When installing a new Solutions Pack, enter the **SECOND MENU** and select the ***PACK USAGE?*** option. Upon answering YES to ***PACK USAGE?***, the EasyLyte analyzer displays and prints the percentage of the Solutions Pack. Press YES again and the EasyLyte analyzer software automatically recognizes and selects the pack size (400mL or 800mL). Answer YES to **RESET TO 0%?** for the Solutions Pack you are installing. The EasyLyte analyzer will then automatically enter *****STANDBY*****. When the EasyLyte analyzer is recalibrated, it will automatically purge the fluid lines of the new Solutions Pack to insure a successful calibration.

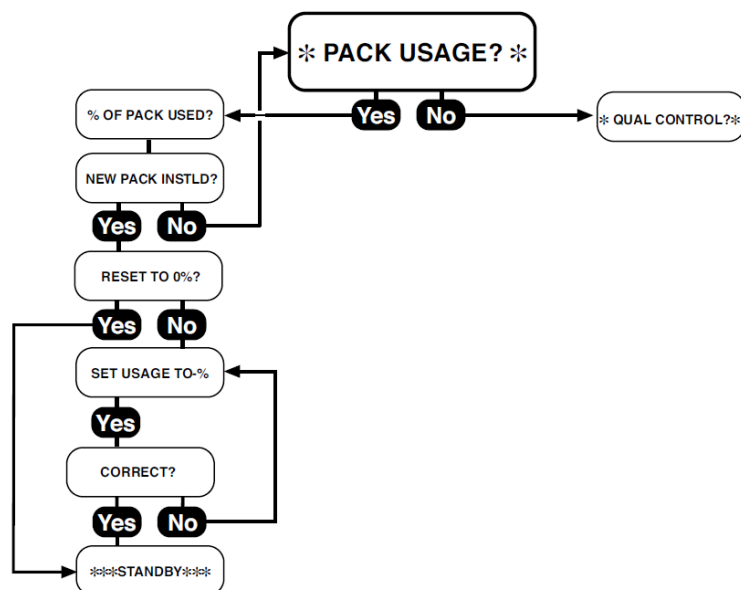

ADDITIONAL INFORMATION

See EasyLyte Operator's Manual for detailed information and performance data.



Medica Corporation, 5 Oak Park Drive
Bedford, MA 01730-1413 USA



Emergo Europe, Prinsessegracht 20
2514 AP The Hague, The Netherlands